


Sleeve Sampler

General


The Sleeve Sampler is designed to take large volume samples from free-flowing powders and granules. The handle can be easily extended to allow samples to be taken from depth.

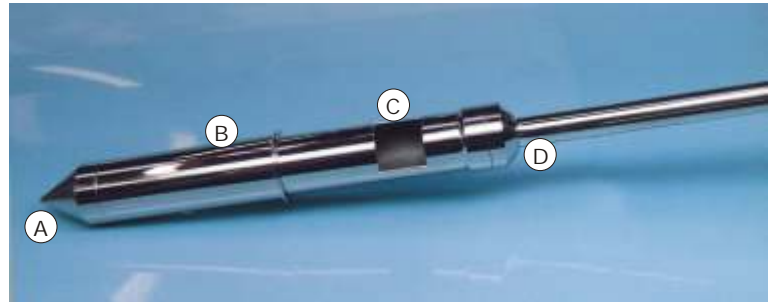

- (A) Tip (screws into chamber)
- (B) Sleeve
- (C) Entrance port for powder
- (D) Chamber screwed to handle to allow different volumes to be attached

Operation

1. Select the correct chamber for the volume to be sampled and screw it onto the handle. Insert the sampler into the product.
2. At the required depth pull up the sampler slightly. This will force the sleeve down so that product can fall into the sample chamber.
3. Remove sampler.
4. To empty sampler either pour sample out of filling port or unscrew the tip.

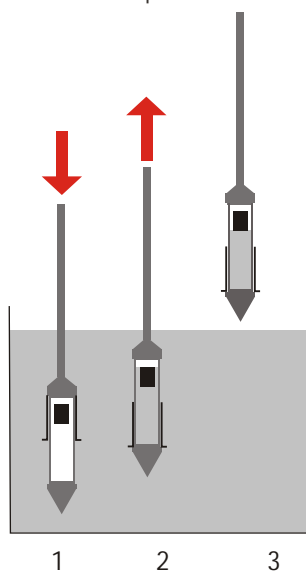

Cleaning

The sampler should be stripped down to its component parts and then cleaned according to the usual cleaning methods that are employed for items such as general dispensing ware, tablet punches etc.

Ensure that the all component parts are thoroughly dried after washing.

Hand Wash ✓	Washing Machine ✓	Ultra-sonic bath ✓	Autoclave 121°C ✓
-------------	-------------------	--------------------	-------------------

IMPORTANT: ENSURE SAMPLER IS CLEANED THOROUGHLY BEFORE INITIAL USE

Whilst every care has been made during the construction of your sampler it should be noted that your new sampler was fabricated and polished in a metal working factory. Ensure that the sampler is thoroughly cleaned according to your normal cleaning procedures and that any polishing waxes have been completely removed before the sampler is used for the first time.

If you have any questions regarding the use of this device please contact Sampling